
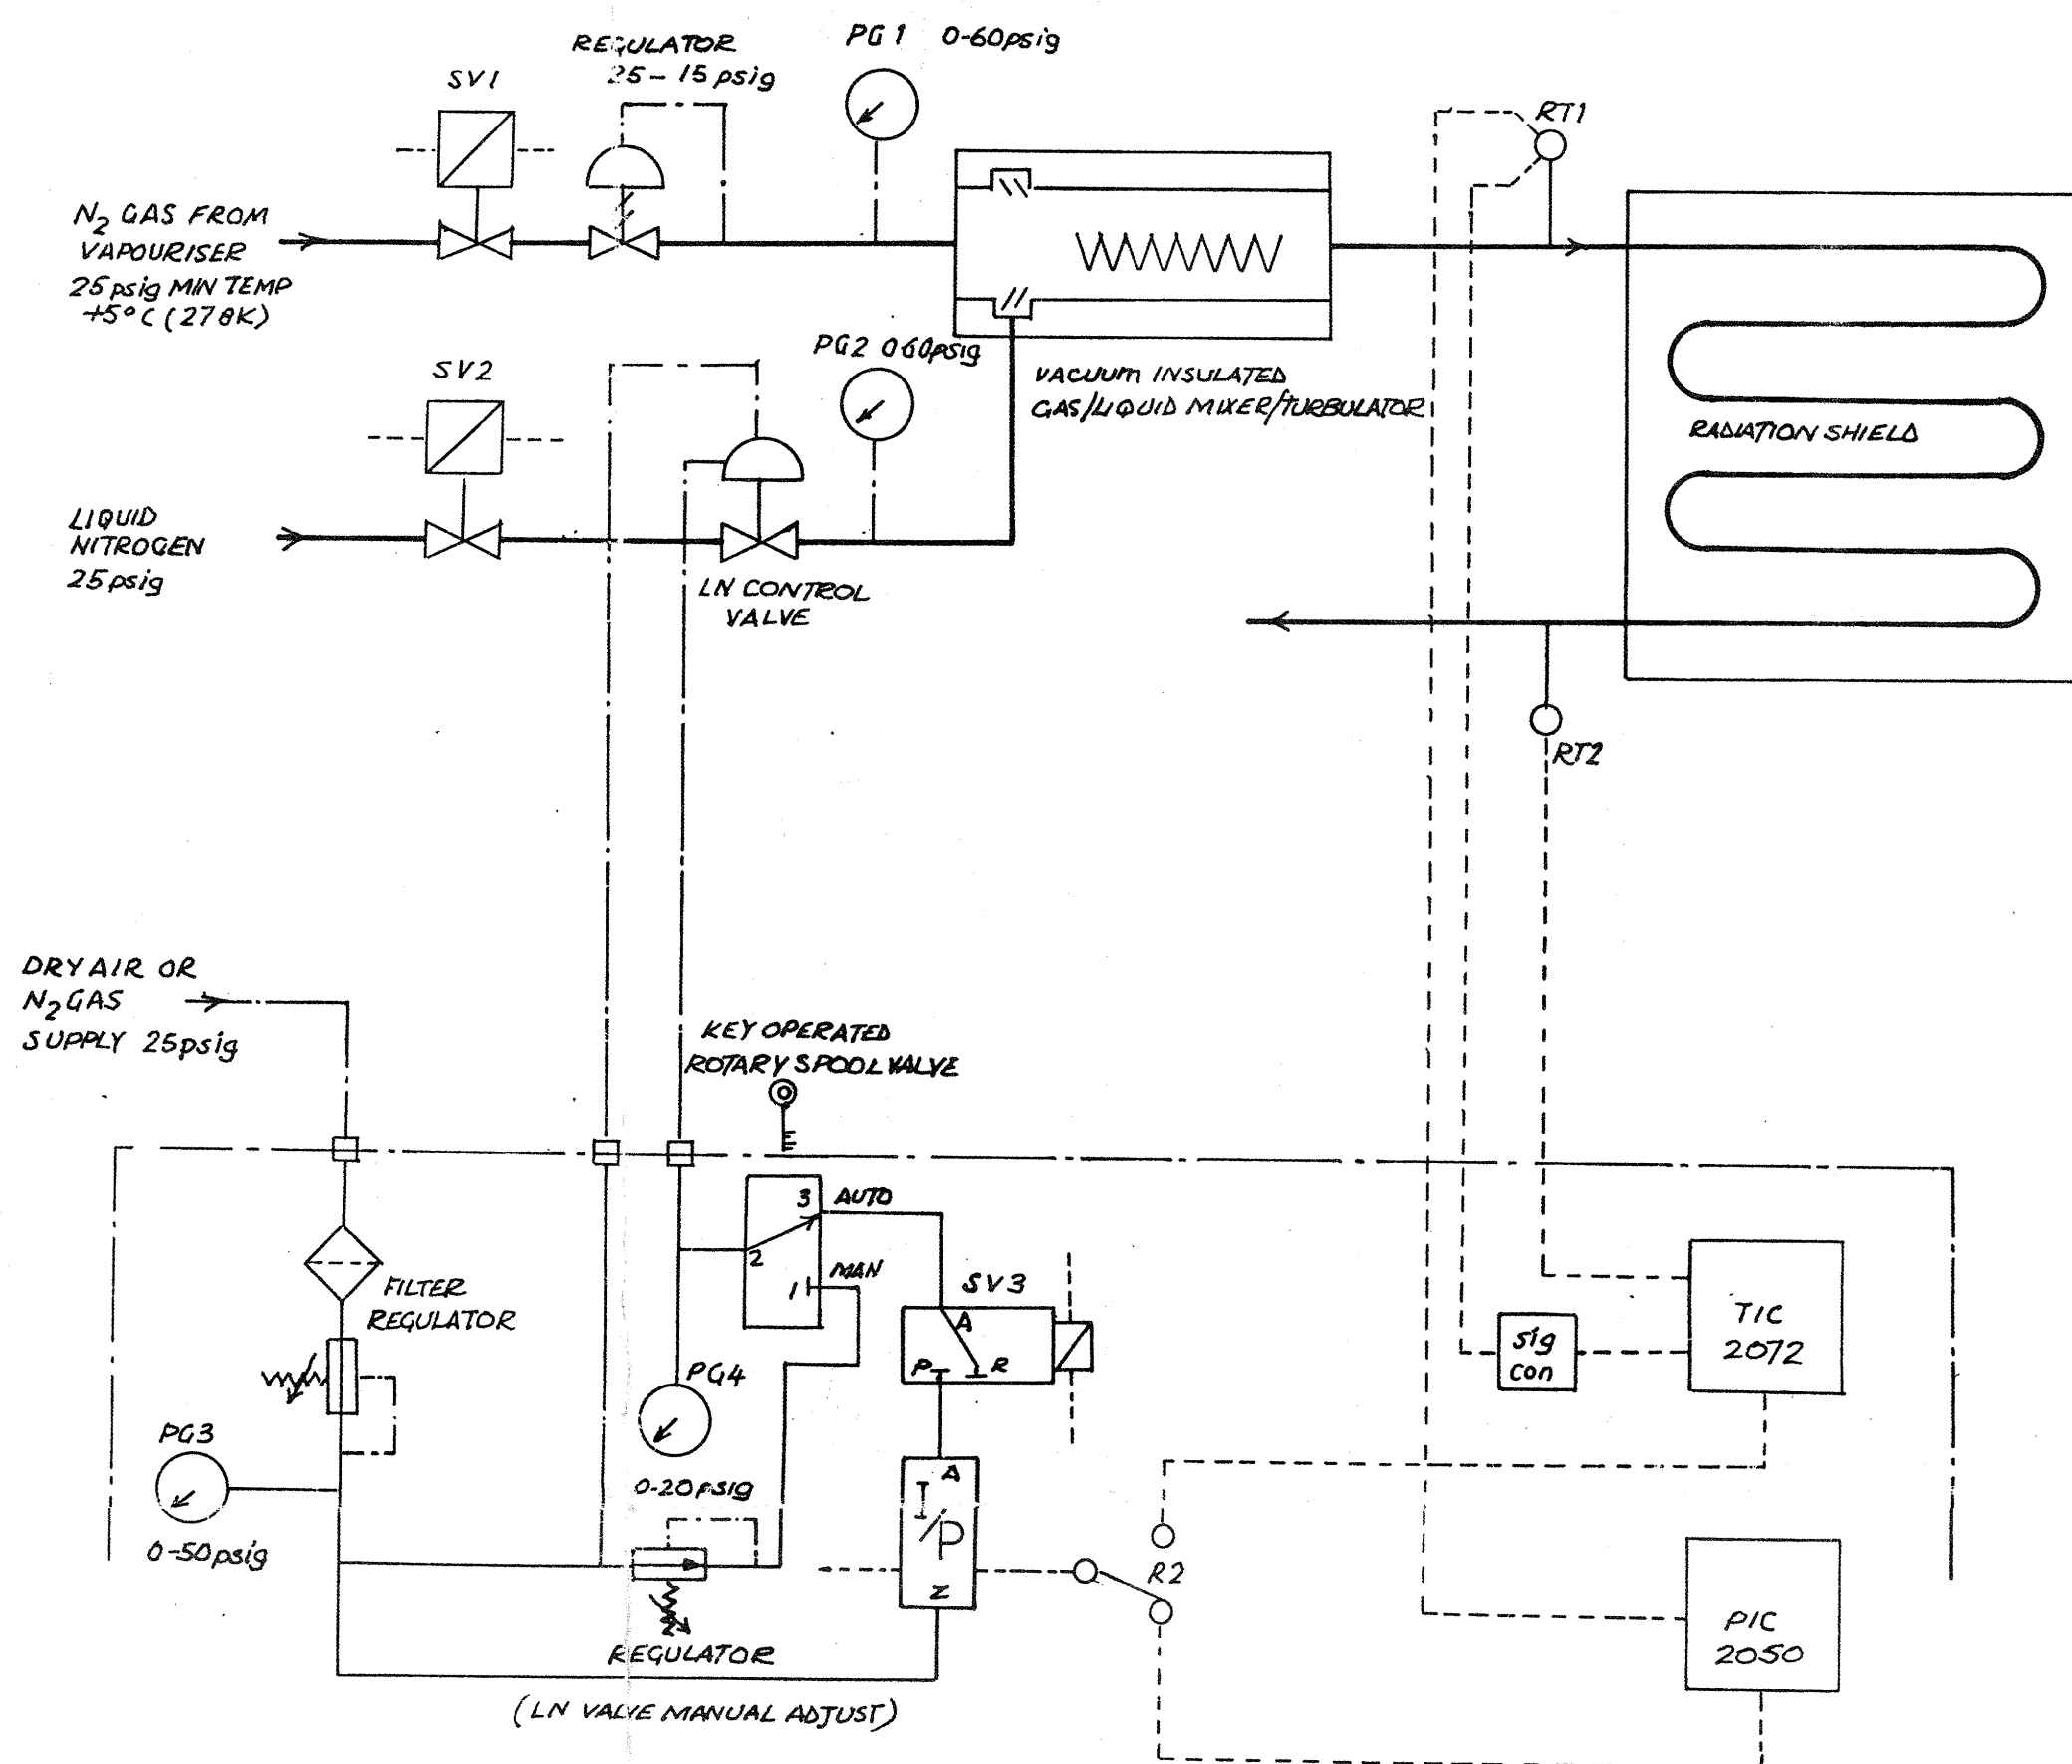


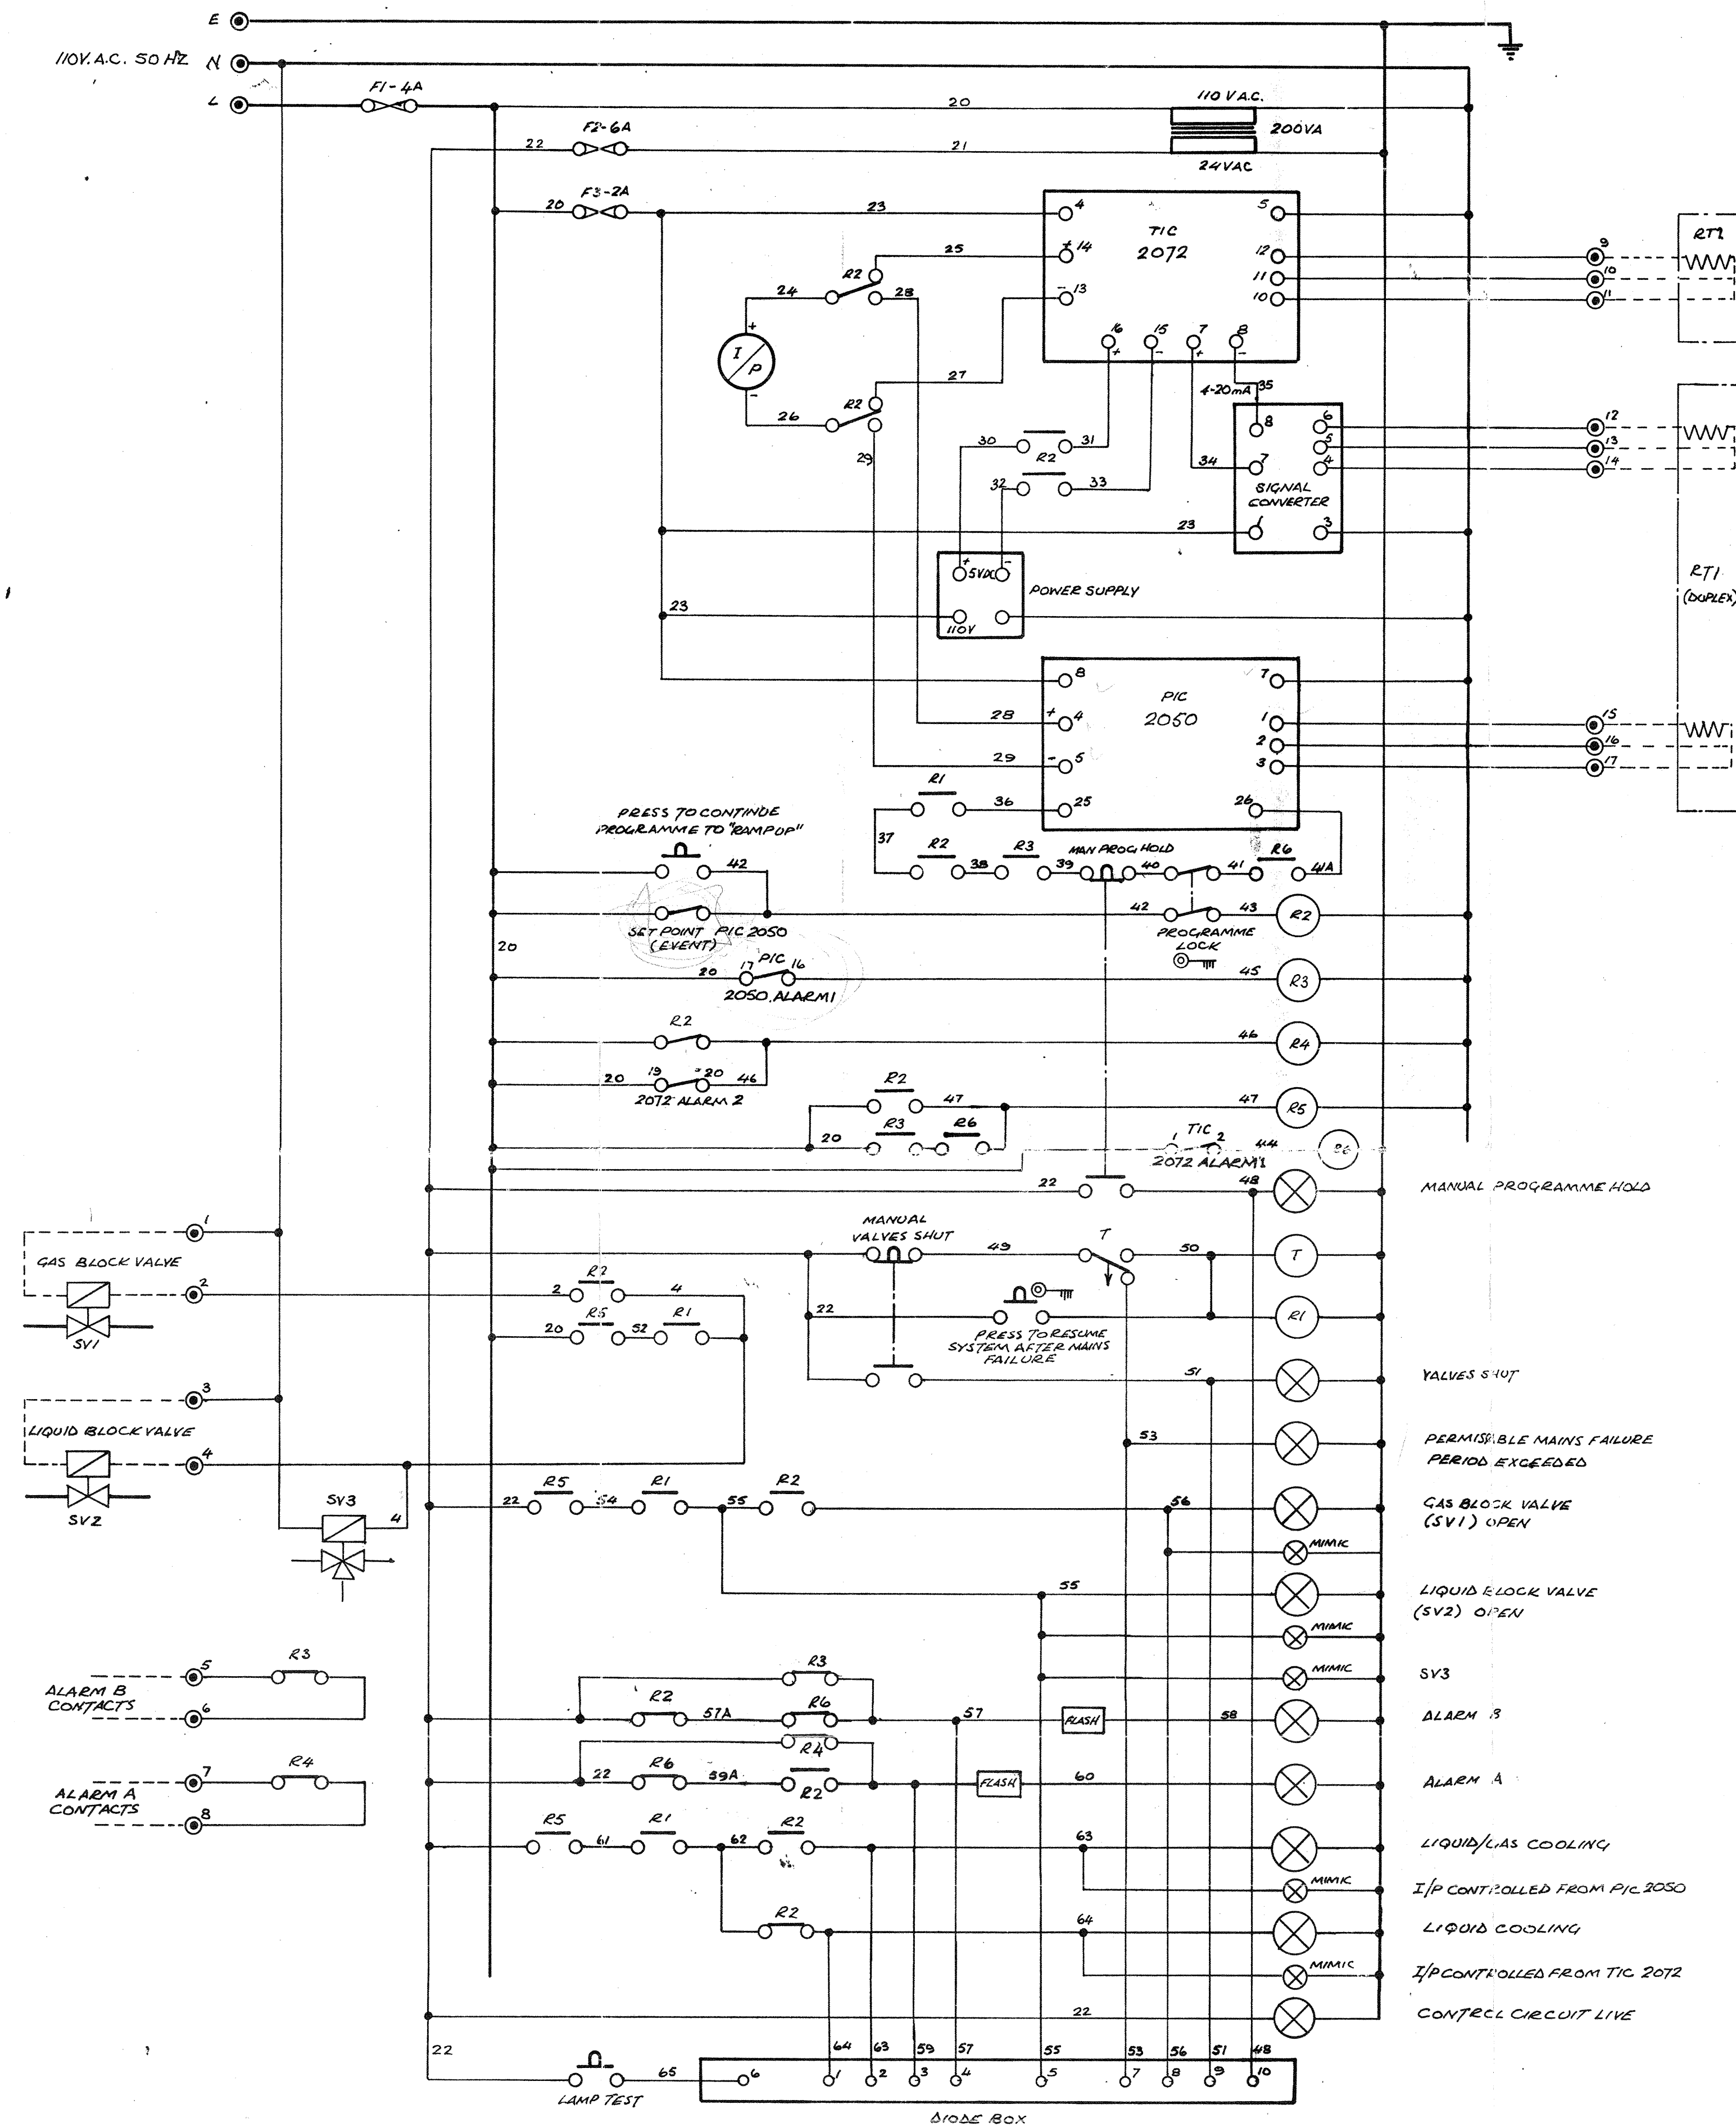

ALARMS	COOLDOWN	STEADY STATE
NO ALARM	LIQUID & GAS BLOCK VALVES OPEN 2050 CONTROLLING LN CONTROL VALVE	LIQUID BLOCK VALVE OPEN 2072 CONTROLLING LN CONTROL VALVE
2050 ALARM 1	ALARM B PROGRAMME HOLD	ALARM B VALVES SHUT
2072 ALARM 1	ALARM A PROGRAMME HOLD	ALARM B VALVES SHUT
2072 ALARM 2	NOTHING NO ACTION	ALARM A NO ACTION

SIGMA ELECTRICAL
ENGINEERING
CONTROL PANELS
BOLTON
(0204) 64322

DRAWN: H.A.H. TRACED: CHECKED: APPROVED: DATE: MAY 1987 SCALE: 1:1

RADIATION SHIELD COOLING SYSTEM - 110V AC.
FOR OXFORD INSTRUMENTS.

BJE 1006

DRAWING No. C1401

No.	DESCRIPTION	CHKD.	APP'D.	DATE
1	ALTERATIONS			

A.S. SCIENTIFIC PRODUCTS LTD
ABBINGTON
A1855