



CERTIFIED CALIBRATION CHART

For Customer
Use Only:

DATE CALIBRATION CYCLE BEGINS

CALIBRATION DUE DATE

MCMaster-CARR SUPPLY CO

KD-10771270

4

CUSTOMER NAME

CUSTOMER ORDER No.

ITEM No.

30326036

4

35W1005PH 02L XC4

300#

ORDER No.

LINE No.

DESCRIPTION

0.

300.

psi

3-2-3%

N/A

E683599

MIN. RANGE

MAX. RANGE

UNITS

ACCURACY

TAG No. / PRODUCT INFO

SERIAL No.

Gauge
Indication

INCREASE

Applied
Pressure

% ERROR

DECREASE

Applied
Pressure

% ERROR

0.00

0.00

0.00%

0.00

0.00%

70.00

69.96

-0.01%

70.86

0.29%

150.00

154.17

1.39%

153.61

1.20%

220.00

224.35

1.45%

223.59

1.20%

300.00

301.16

0.39%

301.16

0.39%

EQUIPMENT USED FOR INSPECTION

Pressure Standard Used :

Ashcroft

Serial /ID Number :

1259

Range :

500 psi

Accuracy :

0.025%

Date Calibrated :


01/25/2022

Due Date of Calibration:

01/25/2023

Tested in accordance with ASME B 40.100:2013
Accuracy of Unit is traceable to N.I.S.T

ERROR - Percent Of Scale Span

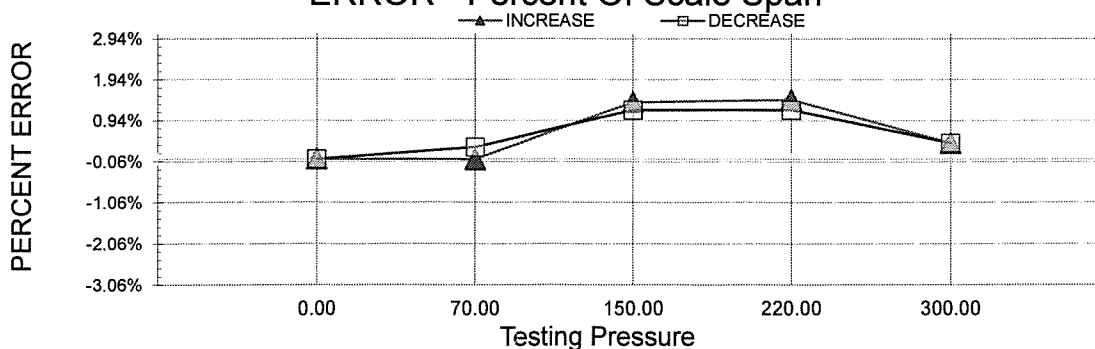

All standards used in this calibration are maintained in accordance with the latest revisions of ANSI/NCSL Z540-1 and ISO-10012

May 8, 2022

8002

Certified By:

Kinga Czyz

DATE OF CALIBRATION
at ASHCROFT® INC.

TESTED BY

Kinga Czyz

This certificate shall not be reproduced, except fully, with a written permission from ASHCROFT® INC.



250 East Main Street - Stratford, CT 06614-5145 - Phone: 203-378-8281 - www.ashcroftinc.com