




CERTIFIED CALIBRATION CHART

For Customer Use Only:	DATE CALIBRATION CYCLE BEGINS	CALIBRATION DUE DATE
---------------------------	-------------------------------	----------------------

MCMaster-CARR SUPPLY CO		KD-10771270		4
CUSTOMER NAME		CUSTOMER ORDER No.		ITEM No.
30326036	4	35W1005PH 02L XC4		300#
ORDER No.	LINE No.	DESCRIPTION		
0.	300.	psi	3-2-3%	N/A
MIN. RANGE	MAX. RANGE	UNITS	ACCURACY	TAG No. / PRODUCT INFO
				E683599
				SERIAL No.

Gauge Indication	INCREASE		DECREASE	
	Applied Pressure	% ERROR	Applied Pressure	% ERROR
0.00	0.00	0.00%	0.00	0.00%
70.00	69.96	-0.01%	70.86	0.29%
150.00	154.17	1.39%	153.61	1.20%
220.00	224.35	1.45%	223.59	1.20%
300.00	301.16	0.39%	301.16	0.39%

EQUIPMENT USED FOR INSPECTION	
Pressure Standard Used :	Ashcroft
Serial /ID Number :	1259
Range :	500 psi
Accuracy :	0.025%
Date Calibrated :	01/25/2022
Due Date of Calibration:	01/25/2023
Tested in accordance with ASME B 40.100:2013 Accuracy of Unit is traceable to N.I.S.T	

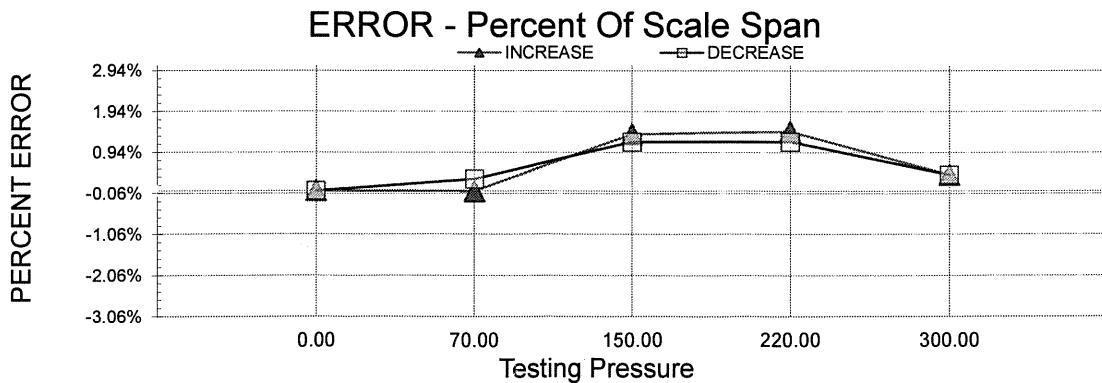

All standards used in this calibration are maintained in accordance with the latest revisions of ANSI/NCSL Z540-1 and ISO-10012

May 8, 2022	8002	Certified By: <i>Kinga Czyz</i>
DATE OF CALIBRATION at ASHCROFT® INC.	TESTED BY	Kinga Czyz

This certificate shall not be reproduced, except fully, with a written permission from ASHCROFT® INC.



250 East Main Street - Stratford, CT 06614-5145 - Phone: 203-378-8281 - www.ashcroftinc.com